


Certificate of CE-Registration

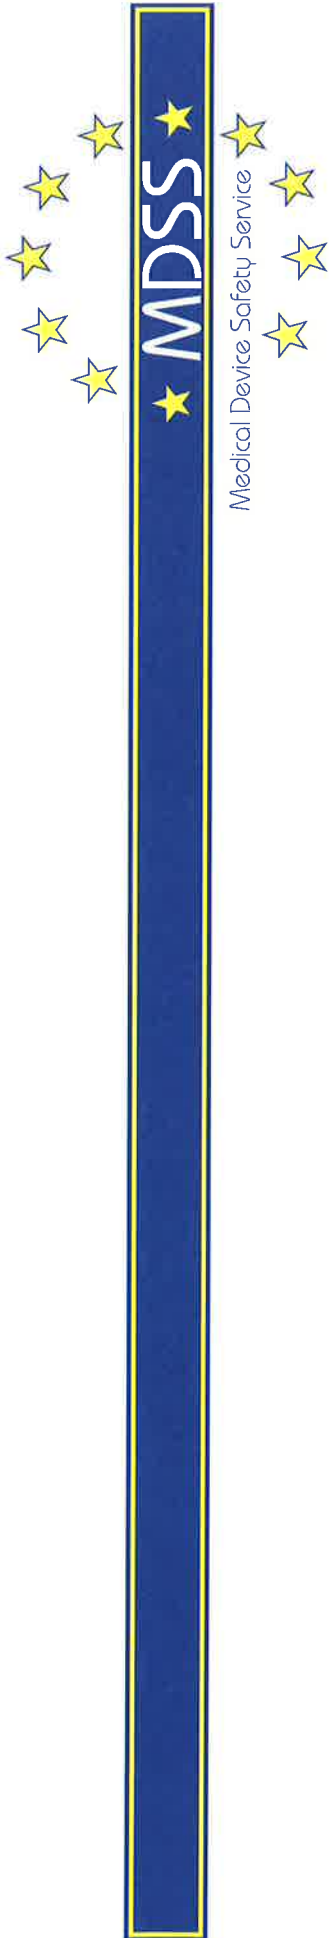

This is to certify that, in accordance with the Medical Device Directive 93/42/EEC, Medical Device Safety Service GmbH (MDSS) agrees to perform all duties and responsibilities as the Authorized Representative for:

**WR Medical Electronics Co.
1700 Gervais Avenue
Maplewood, MN 55109
UNITED STATES OF AMERICA**

as stipulated and demanded by the aforementioned Directive. The German Competent Authority has allocated the medical devices of the Manufacturer registration numbers as foreseen in:

Annex A dated November 23, 2018

The Manufacturer has provided MDSS with the appropriate Declaration(s) of Conformity confirming that the medical devices fulfill the applicable requirements of Directive 93/42/EEC. In compliance with German law, a safety officer has been appointed for Germany.

2018-11-23

Ludger Möller
President
MDSS GmbH

**Annex A dated November 23, 2018
Manufacturer: WR Medical Electronics Co.**

UMDNS Code Description Notified Medical Device Product Name & Catalogue Number	UMDNS Code	Risk Class	Cat. Code	Registration Number	NB No. / NB Certificate No.	NB Cert. Valid Until YYYY-MM-DD
Physiologic Recording Systems Case IV, Q-Sweat	16-306	I m	04	DE/CA09/0170/W07/005-02	0413/41314493-02	2023-10-17
CASE IV™ 5000, 5569 Q-Sweat™ 5188						
Baths, Paraffin, Physical Therapy Therabath® TB6 & TB7	12-956	IIa	05	DE/CA09/0170/W07/004-02	0413/41314493-02	2023-10-17
<i>Therabath TB6, TB7 Part numbers:</i> 2298, 2300, 2302, 2310, 2312, 2320, 2322, 2330, 2332, 2340, 2353, 2354, 2356, 2357, 2373, 2375, 2378, 2379, 2382, 2383, 2389, 2390, 2393, 2395						
Baths, Paraffin, Physical Therapy Therabath Accessories	None	I	05	DE/CA09/0170/1813-Å1	N/A	N/A
<i>Accessories for the Therabath, TB6 & TB7</i> 0100, 0101, 0102, 0107, 0122, 2400, 2401, 2402, 2410, 2411, 2420, 2209, 0205, 0206, 2430, 0130, 0134, 0136, 0138, 0144, 0146, 0148						
Electrodes, other Silverstein, Facial Nerve Monitor/Stimulator,	15-217	I	04	DE/CA09/0170/2713-Å1	N/A	N/A
Cables/Leads Silverstein, Facial Nerve Monitor/Stimulator,	16-312	I	12	DE/CA09/0170/1201-Å2	N/A	N/A
Battery Chargers Silverstein, Facial Nerve Monitor/Stimulator,	17-115	I	12	DE/CA09/0170/1202-Å2	N/A	N/A
Lubricants, Instrument Hilger, Facial Nerve Stimulator Accessory	15-772	I	10	DE/CA09/0170/1444-Å2	N/A	N/A
Physiologic Recording Systems HRV Acquire 5650	16-306	IIa	04	DE/CA09/0170/W07/002-01	0413/41314493-02	2023-10-17
Software WR-TestWorks 5584	26-709	IIa	00	DE/CA09/0170/W07/001-01	0413/41314493-02	2023-10-17

